LOWER LEG SUPPORT INSTRUCTIONS

www.adeptmedical.com

COMPONENTS

PRODUCT CODE
AM3000

- A Foot Plate x 1
- B Leg Pad x 1
- C Lower Leg Support x 1
- D Leg Strap x 3
- E Foot Strap x 2
- F Table Strap x 2

UNBOXING

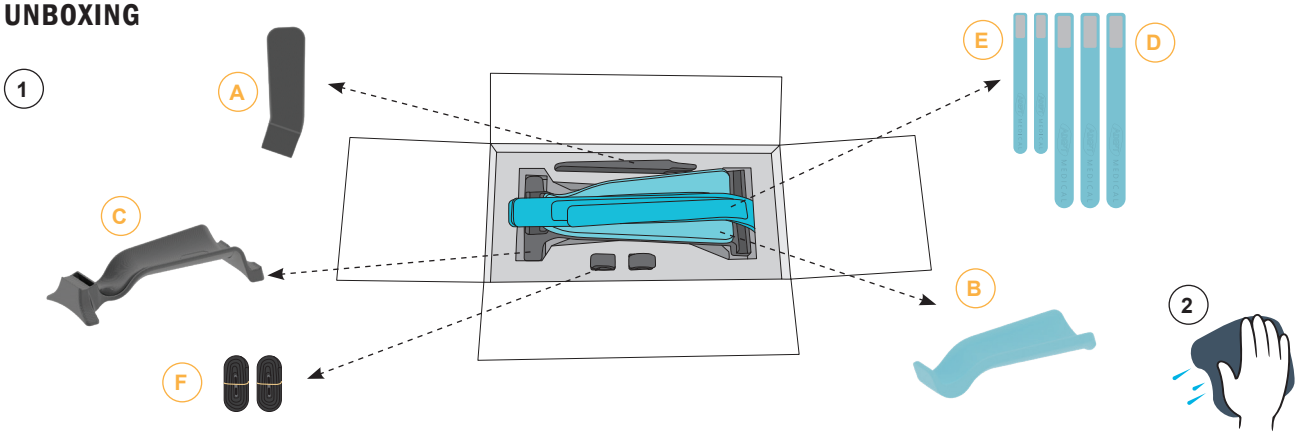

ASSEMBLY

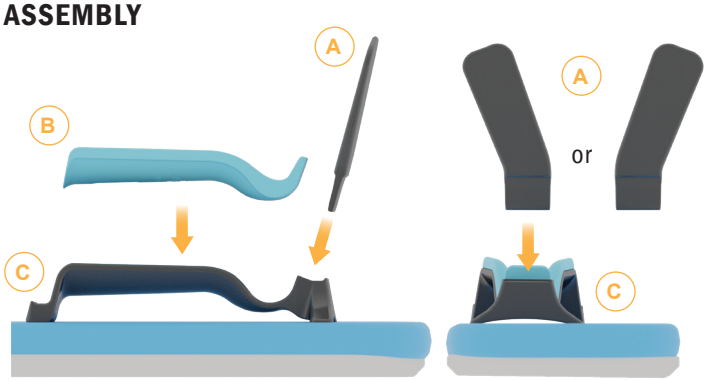

For online training visit:
AdeptMedicalTraining.com

For service and repairs visit:
AdeptMedical.com/repairs

For Approved Disinfectants PDF visit:
AdeptMedicalTraining.com/product-cleaning

CLEANING

Disinfect and wipe clean before/after each use. **DO NOT USE** any other sterilisation methods.

MAXIMUM PATIENT WEIGHT

< 135 kg

MANUFACTURER
Adept Medical Ltd
2-6 McDonald St, Morningside
Auckland 1025, New Zealand
www.adeptmedical.co.nz

EC REPRESENTATIVE
Emergo Europe
Prinsessegracht 20
2514 AP The Hague
The Netherlands

Revision: D | Issue Date: March 2020

LOWER LEG SUPPORT INSTRUCTIONS

www.adeptmedical.com

SETUP | BEFORE PATIENT

Buckle Orientation

Right Leg

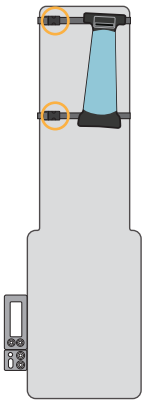

Left Leg

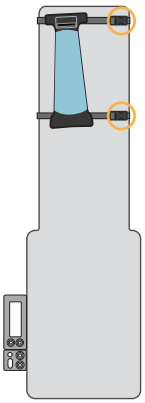

Strap Placement

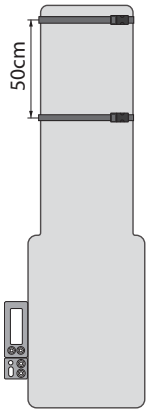

1

2

3 Place the Patient on the Table

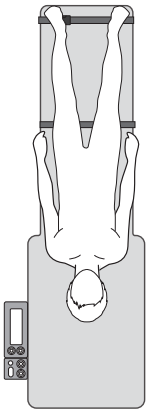

SETUP | PATIENT LEG POSITIONING

1

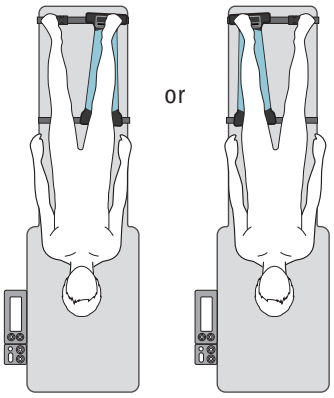

or

2

3

Revision: D | Issue Date: March 2020

LOWER LEG SUPPORT INSTRUCTIONS

www.adeptmedical.com

TIGHTENING TABLE STRAPS

5 Tighten Straps Firmly to Immobilise the Support.

6 Tighten Straps Firmly to Immobilise the Support.

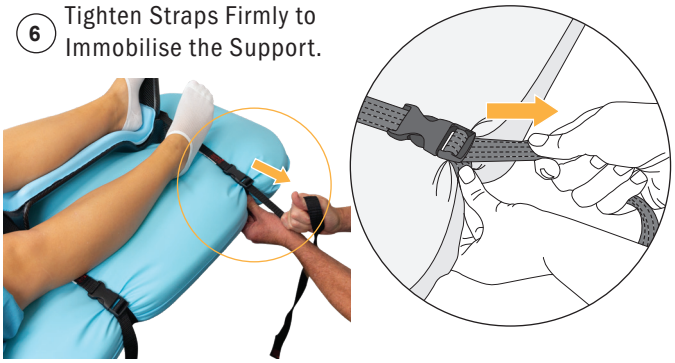

OPTIONAL PADDING (If Required)

Cover Buckles

Supporting the Knee

APPLYING THE STRAPS | LEG STRAPS

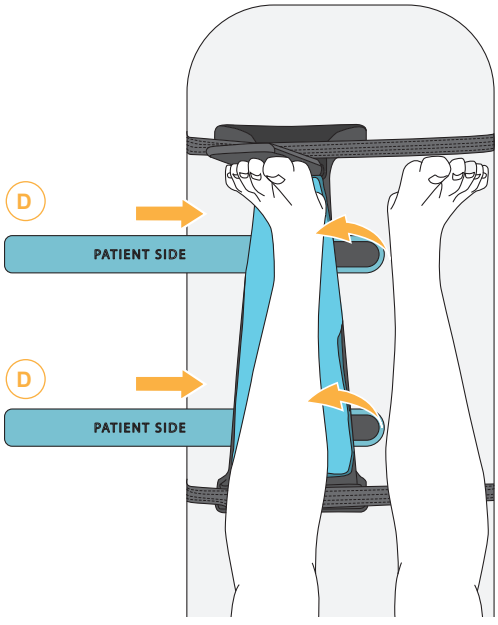

Revision: D | Issue Date: March 2020

APPLYING THE STRAPS | FOOT STRAP

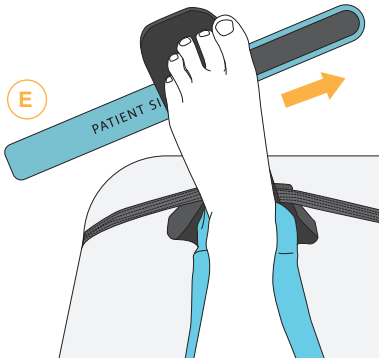

REMOVING THE FOOT PLATE

1

2

FOOTPLATE POSITIONING OPTIONS

Exorotation

or

Endorotation

ACCESSING THE FOOT